

Version 1 Last updated 19 November 2018

ab229406 Human PCSK9 CatchPoint® SimpleStep ELISA® Kit

For the quantitative measurement of PCSK9 in human serum, plasmas, cell culture supernatant, and cell extracts.

This product is for research use only and is not intended for diagnostic use.

Table of Contents

| | |
|-------------------------------------|-----------|
| 1. Overview | 1 |
| 2. Protocol Summary | 2 |
| 3. Precautions | 3 |
| 4. Storage and Stability | 3 |
| 5. Limitations | 4 |
| 6. Materials Supplied | 4 |
| 7. Materials Required, Not Supplied | 5 |
| 8. Technical Hints | 5 |
| 9. Reagent Preparation | 7 |
| 10. Standard Preparation | 8 |
| 11. Sample Preparation | 10 |
| 12. Plate Preparation | 13 |
| 13. Assay Procedure | 14 |
| 14. Calculations | 16 |
| 15. Typical Data | 17 |
| 16. Typical Sample Values | 19 |
| 17. Assay Specificity | 25 |
| 18. Species Reactivity | 25 |
| 19. Troubleshooting | 26 |
| 20. Notes | 27 |
| Technical Support | 30 |

1. Overview

PCSK9 *in vitro* CatchPoint SimpleStep ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for the quantitative measurement of PCSK9 protein in human serum, plasmas, cell culture supernatant, and cell extracts.

The CatchPoint SimpleStep ELISA employs an affinity tag labeled capture antibody and a reporter conjugated detector antibody which immunocapture the sample analyte in solution. This entire complex (capture antibody/analyte/detector antibody) is in turn immobilized via immunoaffinity of an anti-tag antibody coating the well. To perform the assay, samples or standards are added to the wells, followed by the antibody mix. After incubation, the wells are washed to remove unbound material. CatchPoint HRP Development Solution containing the Stoplight Red Substrate is added. During incubation, the substrate is catalyzed by HRP generating a fluorescent product. Signal is generated proportionally to the amount of bound analyte and the intensity is measured in a fluorescence plate reader at 530/570/590 nm Excitation/Cutoff/Emission.

Proprotein convertase subtilisin/kexin type 9 (PCSK9) is a crucial player in the regulation of plasma cholesterol homeostasis. Degradation of low-density lipoprotein receptor family members (LDLR, VLDLR, APOER, and APOER2) is promoted in intracellular acidic compartments following binding by PCSK9.

2. Protocol Summary

Prepare all reagents, samples, and standards as instructed



Add 50 μ L standard or sample to appropriate wells



Add 50 μ L Antibody Cocktail to all wells



Incubate at room temperature for 1 hour



Aspirate and wash each well three times with 350 μ L 1X Wash Buffer
PT



Add 100 μ L of prepared CatchPoint HRP Development Solution to
each well and incubate for 10 minutes



Read fluorescence at Ex/Cutoff/Em 530/570/590 nm

3. Precautions

Please read these instructions carefully prior to beginning the assay.

- All kit components have been formulated and quality control tested to function successfully as a kit.
- We understand that, occasionally, experimental protocols might need to be modified to meet unique experimental circumstances. However, we cannot guarantee the performance of the product outside the conditions detailed in this protocol booklet.
- Reagents should be treated as possible mutagens and should be handled with care and disposed of properly. Please review the Safety Datasheet (SDS) provided with the product for information on the specific components.
- Observe good laboratory practices. Gloves, lab coat, and protective eyewear should always be worn. Never pipet by mouth. Do not eat, drink or smoke in the laboratory areas.
- All biological materials should be treated as potentially hazardous and handled as such. They should be disposed of in accordance with established safety procedures.

4. Storage and Stability

Store kit at +4°C immediately upon receipt. Kit has a storage time of 1 year from receipt, providing components have not been reconstituted.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in the Materials Supplied section.

5. Limitations

- Assay kit intended for research use only. Not for use in diagnostic procedures.
- Do not mix or substitute reagents or materials from other kit lots or vendors. Kits are QC tested as a set of components and performance cannot be guaranteed if utilized separately or substituted.
- All data, except Typical Standard Curve and Sensitivity were collected using the colorimetric version of this kit (ab209884).

6. Materials Supplied

| Item | Quantity | Storage Condition |
|---|----------|-------------------|
| Human PCSK9 Capture Antibody 10X | 600 µL | +4°C |
| Human PCSK9 Detector Antibody 10X | 600 µL | +4°C |
| Human PCSK9 Lyophilized Recombinant Protein | 2 Vials | +4°C |
| Antibody Diluent CPI | 6 mL | +4°C |
| Wash Buffer PT 10X | 20 mL | +4°C |
| Cell Extraction Buffer PTR 5X | 10 mL | +4°C |
| Cell Extraction Enhancer Solution 50X | 1 mL | +4°C |
| Stoptight Red Substrate Buffer | 12 mL | +4°C |
| 100X Stoptight Red Substrate | 120 µL | +4°C |
| 500X Hydrogen Peroxide (H ₂ O ₂ , 3%) | 50 µL | +4°C |
| Sample Diluent NS | 50 mL | +4°C |
| SimpleStep Pre-Coated Black 96-Well Microplate | 96 Wells | +4°C |
| Plate Seal | 1 | +4°C |

7. Materials Required, Not Supplied

These materials are not included in the kit, but will be required to successfully perform this assay:

- Fluorescence microplate reader Ex/Cutoff/Em 530/570/590 nm.
- Method for determining protein concentration (BCA assay recommended).
- Deionized water.
- Multi- and single-channel pipettes.
- Tubes for standard dilution.
- Plate shaker for all incubation steps.
- Optional: Phenylmethylsulfonyl Fluoride (PMSF) (or other protease inhibitors).

8. Technical Hints

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Complete removal of all solutions and buffers during wash steps is necessary to minimize background.
- As a guide, typical ranges of sample concentration for commonly used sample types are shown below in Sample Preparation (section 11).
- All samples should be mixed thoroughly and gently.
- Avoid multiple freeze/thaw of samples.
- Incubate ELISA plates on a plate shaker during all incubation steps.
- When generating positive control samples, it is advisable to change pipette tips after each step.

- The provided Antibody Diluents and Sample Diluents contain protease inhibitor aprotinin. Additional protease inhibitors can be added if required.
- The provided Cell Extraction Buffer 5X contains phosphatase inhibitors and protease inhibitor aprotinin. Additional protease inhibitors can be added if required.
- The provided Cell Extraction Enhancer Solution 50X may precipitate when stored at + 4°C. To dissolve, warm briefly at + 37°C and mix gently. The Cell Extraction Enhancer Solution 50X can be stored at room temperature to avoid precipitation.
- The incubation times provided in this protocol were optimized for fastest results with good signal. It is possible to increase the signal with longer incubation times, further optimization might be necessary.
- Keep in mind any RFU values shown are relative, NOT absolute. RFU from one plate reader are not comparable to another, especially if different make or model.
- **To avoid high background always add samples or standards to the well before the addition of the antibody cocktail.**
- **This kit is sold based on number of tests. A 'test' simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.**

9. Reagent Preparation

- Equilibrate all reagents to room temperature (18-25°C) prior to use. The kit contains enough reagents for 96 wells. The sample volumes below are sufficient for 48 wells (6 x 8-well strips); adjust volumes as needed for the number of strips in your experiment.
- Prepare only as much reagent as is needed on the day of the experiment. Capture and Detector Antibodies have only been tested for stability in the provided 10X formulations.

9.1 1X Cell Extraction Buffer PTR (For cell and tissue extracts only):

Prepare 1X Cell Extraction Buffer PTR by diluting Cell Extraction Buffer PTR 5X to 1X with deionized water. To make 10 mL 1X Cell Extraction Buffer PTR combine 8 mL deionized water and 2 mL Cell Extraction Buffer PTR 5X. Mix thoroughly and gently. If required protease inhibitors can be added.

Alternative – Enhancer may be added to 1X Cell Extraction Buffer PTR after extraction of cells or tissue. Refer to note in the Troubleshooting section.

9.2 1X Wash Buffer PT:

Prepare 1X Wash Buffer PT by diluting Wash Buffer PT 10X with deionized water. To make 50 mL 1X Wash Buffer PT combine 5 mL Wash Buffer PT 10X with 45 mL deionized water. Mix thoroughly and gently.

9.3 Antibody Cocktail:

Prepare Antibody Cocktail by diluting the capture and detector antibodies in Antibody Diluent CPI. To make 3 mL of the Antibody Cocktail combine 300 μ L 10X Capture Antibody and 300 μ L 10X Detector Antibody with 2.4 mL Antibody Diluent CPI. Mix thoroughly and gently.

9.4 CatchPoint HRP Development Solution

Just prior to use prepare CatchPoint HRP Development Solution by diluting the 100X Stoplight Red Substrate and the 500X Hydrogen Peroxide in Stoplight Red Substrate Buffer.

For example, to make 6 mL of the CatchPoint HRP Development Solution combine 60 μ L 100X Stoplight Red Substrate and 12 μ L of 500X Hydrogen Peroxide with 5.928 mL Stoplight Red Substrate Buffer. Mix thoroughly and gently.

10. Standard Preparation

- Always prepare a fresh set of standards for every use.
- Discard working standard dilutions after use as they do not store well.
- The following section describes the preparation of a standard curve for duplicate measurements (recommended).

10.1 For **serum, plasma, and cell culture supernatant** samples, reconstitute the PCSK9 standard by adding 1 mL Sample Diluent NS.

For **cell extract** samples, reconstitute the PCSK9 standard by adding 1 mL 1X Cell Extraction Buffer PTR.

10.2 Mix thoroughly and gently. Hold at room temperature for 10 minutes and mix gently. This is the 40 ng/mL **Stock Standard** Solution.

10.3 Label 11 tubes, Standards 1– 11.

10.4 Add 60 µL appropriate diluent (see step **10.1**) into tube number 1 and 150 µL of appropriate diluent (see step **10.1**) into numbers 2-11.

10.5 Use the Stock Standard to prepare the following dilution series. Standard #11 contains no protein and is the Blank control.

Standards will be added to the plate in step 13.3. If desired all 11 standards can be used for a full standard curve.

Alternatively, to commit fewer wells to the standard curve, select a subset of at least 7 standards plus the blank control. If 7 standards are desired, we recommend standards #1-7.

| Standard # | Dilution Sample | Volume to Dilute (μL) | Volume of Diluent (μL) | Starting Conc. (ng/mL) | Final Conc. (ng/mL) |
|------------|-----------------|-----------------------|------------------------|------------------------|---------------------|
| 1 | Stock | 240 | 60 | 40 | 32 |
| 2 | Standard#1 | 150 | 150 | 32 | 16 |
| 3 | Standard#2 | 150 | 150 | 16 | 8 |
| 4 | Standard#3 | 150 | 150 | 8 | 4 |
| 5 | Standard#4 | 150 | 150 | 4 | 2 |
| 6 | Standard#5 | 150 | 150 | 2 | 1 |
| 7 | Standard#6 | 150 | 150 | 1 | 0.5 |
| 8 | Standard#7 | 150 | 150 | 0.5 | 0.25 |
| 9 | Standard#8 | 150 | 150 | 0.25 | 0.13 |
| 10 | Standard#9 | 150 | 150 | 0.13 | 0.06 |
| 11 | None | 0 | 150 | 0 | 0 |

11. Sample Preparation

| Typical Sample Dynamic Range | |
|--------------------------------|------------------------|
| Sample Type | Range |
| Human Serum | 0.31% - 10% |
| Human Plasma - Citrate | 1.25% - 10% |
| Human Plasma - EDTA | 0.31% - 10% |
| Human Plasma - Heparin | 0.31% - 10% |
| HepG2 Cell Culture Supernatant | 3.13% - 50% |
| HepG2 Cell Extract | 62.5 µg/mL - 500 µg/mL |

11.1 Plasma:

Collect plasma using citrate, EDTA or heparin. Centrifuge samples at 2,000 x g for 10 minutes. Dilute samples into Sample Diluent NS and assay. Store un-diluted plasma samples at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

11.2 Serum:

Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2,000 x g for 10 minutes and collect serum. Dilute samples into Sample Diluent NS and assay. Store un-diluted serum at -20°C or below. Avoid repeated freeze-thaw cycles.

11.3 Cell Culture Supernatants:

Centrifuge cell culture media at 2,000 x g for 10 minutes to remove debris. Collect supernatants and assay. Or dilute samples into Sample Diluent NS and assay. Store un-diluted samples at -20°C or below. Avoid repeated freeze-thaw cycles.

11.4 Preparation of extracts from cell pellets:

- 11.4.1 Collect non-adherent cells by centrifugation or scrape to collect adherent cells from the culture flask. Typical centrifugation conditions for cells are 500 x g for 5 minutes at 4°C.
- 11.4.2 Rinse cells twice with PBS.
- 11.4.3 Solubilize pellet at 2×10^7 cell/mL in chilled 1X Cell Extraction Buffer PTR.
- 11.4.4 Incubate on ice for 20 minutes.
- 11.4.5 Centrifuge at 18,000 x g for 20 minutes at 4°C.
- 11.4.6 Transfer the supernatants into clean tubes and discard the pellets.
- 11.4.7 Assay samples immediately or aliquot and store at -80°C. The sample protein concentration in the extract may be quantified using a protein assay.
- 11.4.8 Dilute samples to desired concentration in 1X Cell Extraction Buffer PTR.

11.5 Preparation of extracts from adherent cells by direct lysis (alternative protocol):

- 11.5.1 Remove growth media and rinse adherent cells 2 times in PBS.
- 11.5.2 Solubilize the cells by addition of chilled 1X Cell Extraction Buffer PTR directly to the plate (use 750 μ L - 1.5 mL 1X Cell Extraction Buffer PTR per confluent 15 cm diameter plate).
- 11.5.3 Scrape the cells into a microfuge tube and incubate the lysate on ice for 15 minutes.
- 11.5.4 Centrifuge at 18,000 x g for 20 minutes at 4°C.
- 11.5.5 Transfer the supernatants into clean tubes and discard the pellets.
- 11.5.6 Assay samples immediately or aliquot and store at -80°C. The sample protein concentration in the extract may be quantified using a protein assay.
- 11.5.7 Dilute samples to desired concentration in 1X Cell Extraction Buffer PTR.

11.6 Preparation of extracts from tissue homogenates:

- 11.6.1 Tissue lysates are typically prepared by homogenization of tissue that is first minced and thoroughly rinsed in PBS to remove blood (dounce homogenizer recommended).
- 11.6.2 Homogenize 100 to 200 mg of wet tissue in 500 μ L – 1 mL of chilled 1X Cell Extraction Buffer PTR. For lower amounts of tissue adjust volumes accordingly.
- 11.6.3 Incubate on ice for 20 minutes.
- 11.6.4 Centrifuge at 18,000 x g for 20 minutes at 4°C.
- 11.6.5 Transfer the supernatants into clean tubes and discard the pellets.
- 11.6.6 Assay samples immediately or aliquot and store at -80°C. The sample protein concentration in the extract may be quantified using a protein assay.
- 11.6.7 Dilute samples to desired concentration in 1X Cell Extraction Buffer PTR.

12. Plate Preparation

- The 96 well plate strips included with this kit are supplied ready to use. It is not necessary to rinse the plate prior to adding reagents.
- Unused plate strips should be immediately returned to the foil pouch containing the desiccant pack, resealed and stored at 4°C.
- For each assay performed, a minimum of two wells must be used as the zero control.
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates).
- Differences in well fluorescence or "edge effects" have not been observed with this assay.
- Ensure plate and all materials are equilibrated to room temperature during use.
- Cover the plate with a plate seal during incubation steps.

13. Assay Procedure

- Equilibrate all materials and prepared reagents to room temperature prior to use.
- We recommend that you assay all standards, controls and samples in duplicate.
- Prepare all reagents, working standards, and samples as directed in the previous sections.

- 13.1** Prepare all reagents, working standards, and samples as directed in the previous sections.
- 13.2** Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, reseal and return to 4°C storage.
- 13.3** Add 50 µL of all sample or standard to appropriate wells.
- 13.4** Add 50 µL of the Antibody Cocktail to each well.
- 13.5** Seal the plate and incubate for 1 hour at room temperature on a plate shaker set to 400 rpm.
- 13.6** Wash each well with 3 x 350 µL 1X Wash Buffer PT. Wash by aspirating or decanting from wells then dispensing 350 µL 1X Wash Buffer PT into each well. Complete removal of liquid at each step is essential for good performance. After the last wash invert the plate and blot it against clean paper towels to remove excess liquid.
- 13.7** Add 100 µL of prepared CatchPoint HRP Development Solution to each well and incubate for 10 minutes in the dark on a plate shaker set to 400 rpm. Further optimization of incubation time vs signal strength can be performed if needed.
- 13.8** Record the fluorescence at Ex/Cutoff/Em 530/570/590 nm. If using a Molecular Devices' plate reader supported by SoftMax® Pro software, a preconfigured protocol for these CatchPoint SimpleStep ELISA Kits is available with all the protocol and analysis settings at www.softmaxpro.org

| | |
|----------------------|----------------------------|
| Mode: | Fluorescence |
| Instrument settings: | Endpoint |
| Excitation: | 530 nm |
| Cutoff: | 570 nm |
| Emission: | 590 nm |
| Sensitivity: | 6 flashes/read or 200ms |
| PMT: | Auto |
| Auto calibrate: | On |
| Read: | Top |
| Read Height: | 1* |

*For microplate readers with Pre-Read Optimization option, the Read Height as well as Microplate Optimization is recommended before the first read.


13.9 Analyze the data as described below.

14. Calculations

- 14.1 Preconfigured protocols are available when using SoftMax Pro software from Molecular Devices
 - 14.2 Calculate the average fluorescence value for the blank control (zero) standards. Subtract the average blank control standard fluorescence value from all other fluorescence values.
 - 14.3 **Create a standard curve** by plotting the average blank control subtracted fluorescence value for each standard concentration (y-axis) against the target protein concentration (x-axis) of the standard. Use graphing software to draw the best smooth curve through these points to construct the standard curve.
- Δ **Note:** Most fluorescence reader software or graphing software will plot these values and fit a curve to the data. A four-parameter curve fit (4PL) is often the best choice; however, other algorithms (e.g. linear, semi-log, log/log, 4-parameter logistic) can also be tested to determine if it provides a better curve fit to the standard values.
- 14.4 Determine the concentration of the target protein in the sample by interpolating the blank control subtracted fluorescence **values against the standard curve**. Multiply the resulting value by the appropriate sample dilution factor, if used, to obtain the concentration of target protein in the sample.
 - 14.5 Samples generating fluorescence values greater than that of the highest standard should be further diluted and reanalyzed. Similarly, samples which measure at fluorescence values less than that of the lowest standard should be retested in a less dilute form.

15. Typical Data

Typical standard curve – data provided **for demonstration purposes only**. A new standard curve must be generated for each assay performed.

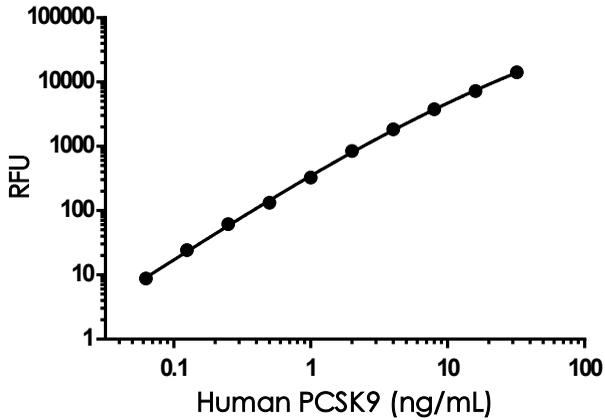

| Standard Curve Measurements | | | |
|-----------------------------|--------|--------|-------------|
| Concentration (ng/mL) | RFU | | Mean RFU |
| | 1 | 2 | |
| 0 | 27 | 27 | 27 |
| 0.06 | 35 | 37 | 36 |
| 0.13 | 49 | 53 | 51 |
| 0.25 | 85 | 94 | 89 |
| 0.5 | 154 | 166 | 160 |
| 1 | 344 | 362 | 353 |
| 2 | 889 | 863 | 876 |
| 4 | 1,895 | 1,828 | 1,862 |
| 8 | 3,788 | 3,786 | 3,787 |
| 16 | 7,359 | 7,165 | 7,262 |
| 32 | 14,146 | 14,161 | 14,153 |

Figure 1. Example of human PCSK9 standard curve in Sample Diluent NS. The PCSK9 standard curve was prepared as described in Section 10. Raw data generated on SpectraMax M4 Multi-Mode Microplate Reader is shown in the table. Background-subtracted data values (mean +/- SD) are graphed.

16. Typical Sample Values

SENSITIVITY –

The calculated minimal detectable dose (MDD) is 37 pg/mL. The MDD was determined by calculating the mean of zero standard replicates (n=16) and adding 2 standard deviations then extrapolating the corresponding concentration.

RECOVERY –

Three concentrations of PCSK9 recombinant protein were spiked in duplicate to the indicated biological matrix to evaluate signal recovery in the working range of the assay.

| Sample Type | Average % Recovery | Range (%) |
|------------------------|--------------------|-----------|
| Human Serum | 105 | 104 - 107 |
| Human Plasma - Citrate | 104 | 102 - 106 |
| Human Plasma - EDTA | 96 | 93 - 100 |
| Human Plasma - Heparin | 111 | 107 - 115 |
| HepG2 Cell Culture | 106 | 103 - 109 |
| HepG2 Cell Extract | 92 | 91 - 94 |

Linearity of Dilution

Linearity of dilution is determined based on interpolated values from the standard curve. Linearity of dilution defines a sample concentration interval in which interpolated target concentrations are directly proportional to sample dilution.

Native PCSK9 was measured in the following biological samples in a 2-fold dilution series. Sample dilutions are made in Sample Diluent NS.

| Dilution Factor | Interpolated value | 10% Human Serum | 10% Human Plasma (Citrate) | 10% Human Plasma (EDTA) | 10% Human Plasma (Heparin) | 50% HepG2 Cell Culture Supernatant |
|-----------------|-------------------------|-----------------|----------------------------|-------------------------|----------------------------|------------------------------------|
| Undiluted | pg/mL | 20.49 | 11.00 | 16.06 | 28.07 | 3.67 |
| | % Expected value | 100 | 100 | 100 | 100 | 100 |
| 2 | pg/mL | 9.90 | 5.53 | 7.84 | 14.11 | 1.72 |
| | % Expected value | 97 | 101 | 98 | 101 | 94 |
| 4 | pg/mL | 5.01 | 2.99 | 4.04 | 6.90 | 0.89 |
| | % Expected value | 98 | 109 | 101 | 98 | 98 |
| 8 | pg/mL | 2.89 | 1.63 | 2.12 | 3.61 | 0.49 |
| | % Expected value | 105 | 119 | 106 | 103 | 106 |
| 16 | pg/mL | 1.32 | NL | 1.18 | 1.87 | 0.25 |
| | % Expected value | 103 | NL | 118 | 107 | 110 |

Native PCSK9 was measured in the following biological samples in a 2-fold dilution series. Sample dilutions are made in 1X Cell Extraction Buffer PTR.

| Dilution Factor | Interpolated value | 500 µg/mL HepG2 Extract |
|-----------------|-------------------------|-------------------------|
| Undiluted | pg/mL | 7.22 |
| | % Expected value | 100 |
| 2 | pg/mL | 3.86 |
| | % Expected value | 107 |
| 4 | pg/mL | 1.96 |
| | % Expected value | 109 |
| 8 | pg/mL | 1.00 |
| | % Expected value | 110 |

PRECISION –

Mean coefficient of variations of interpolated values of PCSK9 from three concentrations of pooled normal human serum within the working range of the assay.

| | Intra-Assay | Inter-Assay |
|-------|-------------|-------------|
| n = | 5 | 3 |
| CV(%) | 4.4 | 4.6 |

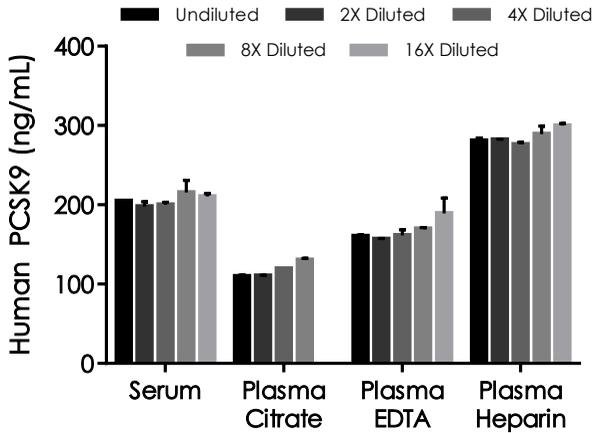


Figure 2. Interpolated concentrations of native PCSK9 in human serum and plasma samples. The concentrations of PCSK9 were measured in duplicates, interpolated from the PCSK9 standard curves and corrected for sample dilution. Undiluted samples are as follows: serum 10%, plasma (citrate) 10%, and plasma (heparin) 10%. The interpolated dilution factor corrected values are plotted (mean +/- SD, n=2). The mean PCSK9 concentration was determined to be 207 ng/mL in serum, 117 ng/mL in plasma (citrate), 166 ng/mL in plasma (EDTA), and 292 ng/mL in plasma (heparin).

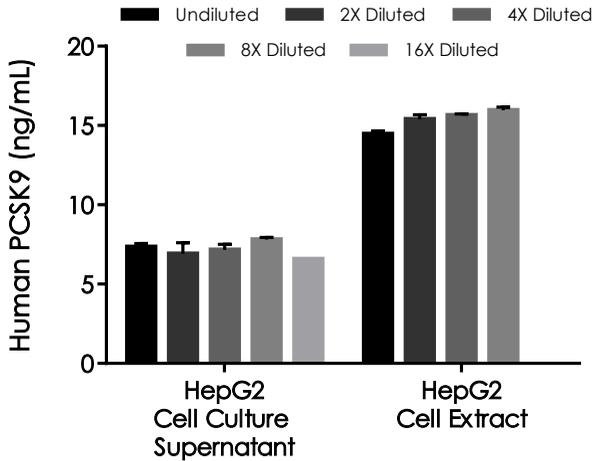


Figure 3. Interpolated concentrations of native PCSK9 in HepG2 cell culture supernatant and cell extract. The concentrations of PCSK9 were measured in duplicate, interpolated from the PCSK9 standard curve, and corrected for sample dilution. Undiluted samples are as follows: HepG2 cell culture supernatant 50%, HepG2 cell extract 500 µg/mL. The interpolated dilution factor corrected values are plotted (mean +/- SD, n=2). The mean PCSK9 concentration was determined to be 7.3 ng/mL in HepG2 cell culture supernatant and 15 ng/mL in HepG2 cell extract.

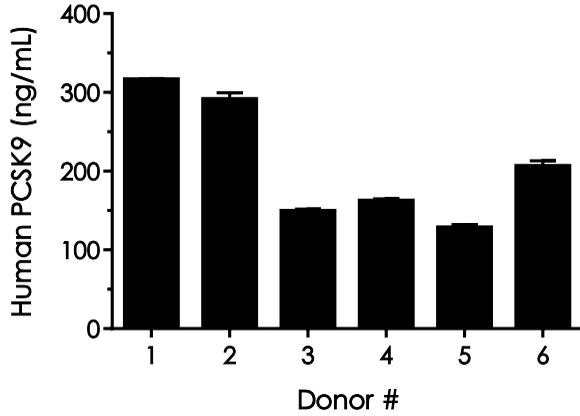


Figure 4. Serum from six individual human male donors was measured in duplicate. Interpolated dilution factor corrected values are plotted (mean \pm SD, n=2). The mean PCSK9 concentration was determined to be 208 ng/mL with a range of 125 - 317 ng/mL.

17. Assay Specificity

This kit recognizes both native and recombinant human PCSK9 protein in serum, plasma, cell culture supernatant, cell extract samples only. This assay uses a recombinant fragment (31 kD) for the kit standard and has been calibrated against the full-length recombinant protein.

INTERFERENCE

Interference was not observed in 10% normal human serum when spiked with 4 ng/mL recombinant LDLR.

18. Species Reactivity

This kit recognizes human PCSK9 protein.

Other species reactivity was determined by measuring 10% serum samples of various species, interpolating the protein concentrations from the human standard curve, and expressing the interpolated concentrations as a percentage of the protein concentration in human serum assayed at the same dilution.

Reactivity < 3% was determined for the following species:

- Mouse
- Rat
- Cow

Please contact our Technical Support team for more information.

19. Troubleshooting

| Problem | Reason | Solution |
|---|---|---|
| Difficulty pipetting lysate; viscous lysate. | Genomic DNA solubilized | Prepare 1X Cell Extraction Buffer PTR (without enhancer). Add enhancer to lysate after extraction. |
| Poor standard curve | Inaccurate Pipetting | Check pipettes |
| | Improper standard dilution | Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing |
| Low Signal | Incubation times too brief | Ensure sufficient incubation times; increase to 2 or 3 hour standard/sample incubation |
| | Inadequate reagent volumes or improper dilution | Check pipettes and ensure correct preparation |
| | Incubation times with CatchPoint HRP Development Solution too brief | Read plate again after longer incubation time |
| Large CV | Plate is insufficiently washed | Review manual for proper wash technique. If using a plate washer, check all ports for obstructions. |
| | Contaminated wash buffer | Prepare fresh wash buffer |
| Low sensitivity | Improper storage of the ELISA kit | Store your reconstituted standards at -80°C, all other assay components 4°C. Keep Stoplight Red Substrate protected from light. |
| Precipitate in Diluent | Precipitation and/or coagulation of components within the Diluent. | Precipitate can be removed by gently warming the Diluent to 37°C. |

20. Notes

Technical Support

Copyright © 2018 Abcam, All Rights Reserved. The Abcam logo is a registered trademark. All information / detail is correct at time of going to print. This product was released in collaboration with Molecular Devices LLC, however for technical support questions, please contact Abcam Representatives.

Austria

wissenschaftlicherdienst@abcam.com | 019-288-259

France

supportscientifique@abcam.com | 01.46.94.62.96

Germany

wissenschaftlicherdienst@abcam.com | 030-896-779-154

Spain

soportecientifico@abcam.com | 91-114-65-60

Switzerland

technical@abcam.com

Deutsch: 043-501-64-24 | Français: 061-500-05-30

UK, EU and ROW

technical@abcam.com | +44(0)1223-696000

Canada

ca.technical@abcam.com | 877-749-8807

US and Latin America

us.technical@abcam.com | 888-772-2226

Asia Pacific

hk.technical@abcam.com | (852) 2603-6823

China

cn.technical@abcam.com | 400 921 0189 / +86 21 2070 0500

Japan

technical@abcam.co.jp | +81-(0)3-6231-0940

Singapore

sg.technical@abcam.com | 800 188-5244

Australia

au.technical@abcam.com | +61-(0)3-8652-1450

New Zealand

nz.technical@abcam.com | +64-(0)9-909-7829