

Version 1 Last updated 19 November 2018

ab229413 Human GLP-1 (7-36) CatchPoint[®] SimpleStep ELISA[®] Kit

For the quantitative measurement of GLP-1 (7-36) in human serum, plasma, and cell culture supernatants.

This product is for research use only and is not intended for diagnostic use.

Table of Contents

1. Overview	1
2. Protocol Summary	3
3. Precautions	4
4. Storage and Stability	4
5. Limitations	5
6. Materials Supplied	5
7. Materials Required, Not Supplied	6
8. Technical Hints	6
9. Reagent Preparation	8
10. Standard Preparation	9
11. Sample Preparation	11
12. Plate Preparation	12
13. Assay Procedure	13
14. Calculations	15
15. Typical Data	16
16. Typical Sample Values	18
17. Assay Specificity	21
18. Species Reactivity	21
19. Troubleshooting	22
20. Notes	23
Technical Support	26

1. Overview

GLP-1 (7-36) *in vitro* CatchPoint SimpleStep ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for the quantitative measurement of GLP-1 (7-36) protein in human serum, plasma, and cell culture supernatants.

The CatchPoint SimpleStep ELISA employs an affinity tag labeled capture antibody and a reporter conjugated detector antibody which immunocapture the sample analyte in solution. This entire complex (capture antibody/analyte/detector antibody) is in turn immobilized via immunoaffinity of an anti-tag antibody coating the well. To perform the assay, samples or standards are added to the wells, followed by the antibody mix. After incubation, the wells are washed to remove unbound material. CatchPoint HRP Development Solution containing the Stoplight Red Substrate is added. During incubation, the substrate is catalyzed by HRP generating a fluorescent product. Signal is generated proportionally to the amount of bound analyte and the intensity is measured in a fluorescence plate reader at 530/570/590 nm Excitation/Cutoff/Emission.

GLP-1 (Glucagon like peptide 1) is part of the group of incretin hormones that are secreted by the gastrointestinal tract in response to food intake to assist glucose stimulated insulin secretion and glucagon suppression. GLP-1 is a 30 amino acid peptide cleaved from proglucagon and released by the L-cells of the distal ileum. The intracellular precursor of GLP-1 (1-37) is cleaved to form the active peptides GLP-1 (7-37) and GLP-1 (7-36)NH₂. The active peptides bind to the GLP-1 receptor (GLP-1r) expressed in the pancreatic beta cell and are quickly metabolized by the enzyme dipeptidyl peptidase IV (DPP-IV) to form the peptide GLP-1 (9-36), which has no insulin stimulating activity. Binding of active GLP-1 to the receptor, increases cAMP levels and potentiates insulin secretion via Protein Kinase A (PKA) and the cAMP-regulated nucleotide exchange factor (Epac2). GLP-1 and its receptor are also suggested to play a role in the central nervous systems as mediators of satiety. Intracerebroventricular GLP-1 has been shown to induce c-FOS activity in the hypothalamus and the central nucleus of the

amygdala, both of which are important in the regulation of appetite.

The role of GLP-1 in chronic diseases is controversial. Patients with type-II diabetes as well as morbidly obese subjects have been shown to have lower secretion of post-prandial GLP-1, which improves with treatment or weight loss. Due to the beneficial effects of active GLP-1 as well as GLP-1r agonists in metabolic diseases, GLP-1 has been proposed to be an effective therapeutic approach to lowering glycemic levels and decreasing body fat content. Furthermore, GLP-1 has been found to be cardioprotective during acute myocardial infarction. In contrast with the GLP-1 protective findings, circulating GLP-1 has also been found to positively correlate with serum triglycerides and high levels are significantly associated with coronary plaque burden in patients receiving coronary CT-angiography.

2. Protocol Summary

Prepare all reagents, samples, and standards as instructed



Add 50 μ L standard or sample to appropriate wells



Add 50 μ L Antibody Cocktail to all wells



Incubate at room temperature for 1 hour



Aspirate and wash each well three times with 350 μ L 1X Wash Buffer
PT



Add 100 μ L of prepared CatchPoint HRP Development Solution to
each well and incubate for 15 minutes



Read fluorescence at Ex/Cutoff/Em 530/570/590 nm

3. Precautions

Please read these instructions carefully prior to beginning the assay.

- All kit components have been formulated and quality control tested to function successfully as a kit.
- We understand that, occasionally, experimental protocols might need to be modified to meet unique experimental circumstances. However, we cannot guarantee the performance of the product outside the conditions detailed in this protocol booklet.
- Reagents should be treated as possible mutagens and should be handled with care and disposed of properly. Please review the Safety Datasheet (SDS) provided with the product for information on the specific components.
- Observe good laboratory practices. Gloves, lab coat, and protective eyewear should always be worn. Never pipet by mouth. Do not eat, drink or smoke in the laboratory areas.
- All biological materials should be treated as potentially hazardous and handled as such. They should be disposed of in accordance with established safety procedures.

4. Storage and Stability

Store kit at +4°C immediately upon receipt. Kit has a storage time of 1 year from receipt, providing components have not been reconstituted.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in the Materials Supplied section.

5. Limitations

- Assay kit intended for research use only. Not for use in diagnostic procedures.
- Do not mix or substitute reagents or materials from other kit lots or vendors. Kits are QC tested as a set of components and performance cannot be guaranteed if utilized separately or substituted.
- All data, except Typical Standard Curve and Sensitivity were collected using the colorimetric version of this kit (ab184857).

6. Materials Supplied

Item	Quantity	Storage Condition
Human GLP-1 (7-36) Capture Antibody 10X	600 µL	+4°C
Human GLP-1 (7-36) Detector Antibody 10X	600 µL	+4°C
Human GLP-1 (7-36) Lyophilized Recombinant Protein	2 Vials	+4°C
Antibody Diluent CPI	6 mL	+4°C
Wash Buffer PT 10X	20 mL	+4°C
Stoplight Red Substrate Buffer	12 mL	+4°C
100X Stoplight Red Substrate	120 µL	+4°C
500X Hydrogen Peroxide (H ₂ O ₂ , 3%)	50 µL	+4°C
Sample Diluent NS	50 mL	+4°C
SimpleStep Pre-Coated Black 96-Well Microplate	96 Wells	+4°C
Plate Seal	1	+4°C

7. Materials Required, Not Supplied

These materials are not included in the kit, but will be required to successfully perform this assay:

- Fluorescence microplate reader Ex/Cutoff/Em 530/570/590 nm.
- Method for determining protein concentration (BCA assay recommended).
- Deionized water.
- Multi- and single-channel pipettes.
- Tubes for standard dilution.
- Plate shaker for all incubation steps.
- Optional: Phenylmethylsulfonyl Fluoride (PMSF) (or other protease inhibitors).

8. Technical Hints

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Complete removal of all solutions and buffers during wash steps is necessary to minimize background.
- As a guide, typical ranges of sample concentration for commonly used sample types are shown below in Sample Preparation (section 11).
- All samples should be mixed thoroughly and gently.
- Avoid multiple freeze/thaw of samples.
- Incubate ELISA plates on a plate shaker during all incubation steps.
- When generating positive control samples, it is advisable to change pipette tips after each step.

- The provided Antibody Diluents and Sample Diluents contain protease inhibitor aprotinin. Additional protease inhibitors can be added if required.
- The incubation times provided in this protocol were optimized for fastest results with good signal. It is possible to increase the signal with longer incubation times, further optimization might be necessary.
- Keep in mind any RFU values shown are relative, NOT absolute. RFU from one plate reader are not comparable to another, especially if different make or model.
- **To avoid high background always add samples or standards to the well before the addition of the antibody cocktail.**
- **This kit is sold based on number of tests. A 'test' simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.**

9. Reagent Preparation

- Equilibrate all reagents to room temperature (18-25°C) prior to use. The kit contains enough reagents for 96 wells. The sample volumes below are sufficient for 48 wells (6 x 8-well strips); adjust volumes as needed for the number of strips in your experiment.
- Prepare only as much reagent as is needed on the day of the experiment. Capture and Detector Antibodies have only been tested for stability in the provided 10X formulations.

9.1 1X Wash Buffer PT:

Prepare 1X Wash Buffer PT by diluting Wash Buffer PT 10X with deionized water. To make 50 mL 1X Wash Buffer PT combine 5 mL Wash Buffer PT 10X with 45 mL deionized water. Mix thoroughly and gently.

9.2 Antibody Cocktail:

Prepare Antibody Cocktail by diluting the capture and detector antibodies in Antibody Diluent CPI. To make 3 mL of the Antibody Cocktail combine 300 μ L 10X Capture Antibody and 300 μ L 10X Detector Antibody with 2.4 mL Antibody Diluent CPI. Mix thoroughly but **very** gently. Do not vortex and take care not to generate any bubbles while mixing.

9.3 CatchPoint HRP Development Solution

Just prior to use prepare CatchPoint HRP Development Solution by diluting the 100X Stoplight Red Substrate and the 500X Hydrogen Peroxide in Stoplight Red Substrate Buffer.

For example, to make 6 mL of the CatchPoint HRP Development Solution combine 60 μ L 100X Stoplight Red Substrate and 12 μ L of 500X Hydrogen Peroxide with 5.928 mL Stoplight Red Substrate Buffer. Mix thoroughly and gently.

10. Standard Preparation

- Always prepare a fresh set of standards for every use.
- Discard working standard dilutions after use as they do not store well.
- The following section describes the preparation of a standard curve for duplicate measurements (recommended).

10.1 Reconstitute the GLP-1 (7-36) standard sample by adding 1,000 μ L Sample Diluent NS. Mix thoroughly and gently. Hold at room temperature for 10 minutes and mix gently. This is the 1,000 pg/mL **Stock Standard** Solution.

10.2 Label 10 tubes, Standards 2– 11. The **Stock Standard** solution will be standard #1.

10.3 Add 225 μ L of Sample Diluent NS into numbers 2-11.

10.4 Use the Stock Standard to prepare the following dilution series. Standard #11 contains no protein and is the Blank control.

Standards will be added to the plate in step 13.3. If desired all 11 standards can be used for a full standard curve.

Alternatively, to commit fewer wells to the standard curve, select a subset of at least 7 standards plus the blank control. If 7 standards are desired, we recommend standards #1-7.

Standard #	Dilution Sample	Volume to Dilute (μL)	Volume of Diluent (μL)	Starting Conc. (pg/mL)	Final Conc. (pg/mL)
1	Stock				1,000
2	Standard#1	375	225	1,000	625
3	Standard#2	375	225	625	390.6
4	Standard#3	375	225	390.6	244.1
5	Standard#4	375	225	244.1	152.6
6	Standard#5	375	225	152.6	95.4
7	Standard#6	375	225	95.4	59.6
8	Standard#7	375	225	59.6	37.3
9	Standard#8	375	225	37.3	23.3
10	Standard#9	375	225	23.3	14.6
11	None	0	225	0	0

11. Sample Preparation

Typical Sample Dynamic Range	
Sample Type	Range
Culture Media	1 – 10%
Human Serum	1 – 10%
Human Plasma - Heparin	0.1 – 1%
Human Plasma - Citrate	1 – 10%
Human Plasma - EDTA	Not recommended

11.1 Plasma:

Collect plasma using citrate or heparin. Centrifuge samples at 2,000 x g for 10 minutes. Dilute samples into Sample Diluent NS and assay. Store un-diluted plasma samples at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

11.2 Serum:

Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2,000 x g for 10 minutes and collect serum. Dilute samples into Sample Diluent NS and assay. Store un-diluted serum at -20°C or below. Avoid repeated freeze-thaw cycles.

11.3 Cell Culture Supernatants:

Centrifuge cell culture media at 2,000 x g for 10 minutes to remove debris. Collect supernatants and assay. Or dilute samples into Sample Diluent NS and assay. Store un-diluted samples at -20°C or below. Avoid repeated freeze-thaw cycles.

12. Plate Preparation

- The 96 well plate strips included with this kit are supplied ready to use. It is not necessary to rinse the plate prior to adding reagents.
- Unused plate strips should be immediately returned to the foil pouch containing the desiccant pack, resealed and stored at 4°C.
- For each assay performed, a minimum of two wells must be used as the zero control.
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates).
- Differences in well fluorescence or "edge effects" have not been observed with this assay.
- Ensure plate and all materials are equilibrated to room temperature during use.
- Cover the plate with a plate seal during incubation steps.

13. Assay Procedure

- Equilibrate all materials and prepared reagents to room temperature prior to use.
 - We recommend that you assay all standards, controls and samples in duplicate.
 - Prepare all reagents, working standards, and samples as directed in the previous sections.
- 13.1** Prepare all reagents, working standards, and samples as directed in the previous sections.
 - 13.2** Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, reseal and return to 4°C storage.
 - 13.3** Add 50 µL of all sample or standard to appropriate wells.
 - 13.4** Add 50 µL of the Antibody Cocktail to each well.
 - 13.5** Seal the plate and incubate for 1 hour at room temperature on a plate shaker set to 400 rpm.
 - 13.6** Wash each well with 3 x 350 µL 1X Wash Buffer PT. Wash by aspirating or decanting from wells then dispensing 350 µL 1X Wash Buffer PT into each well. Complete removal of liquid at each step is essential for good performance. After the last wash invert the plate and blot it against clean paper towels to remove excess liquid.
 - 13.7** Add 100 µL of prepared CatchPoint HRP Development Solution to each well and incubate for 15 minutes in the dark on a plate shaker set to 400 rpm. Further optimization of incubation time vs signal strength can be performed if needed.
 - 13.8** Record the fluorescence at Ex/Cutoff/Em 530/570/590 nm. If using a Molecular Devices' plate reader supported by SoftMax® Pro software, a preconfigured protocol for these CatchPoint SimpleStep ELISA Kits is available with all the protocol and analysis settings at www.softmaxpro.org

Mode:	Fluorescence
Instrument settings:	Endpoint
Excitation:	530 nm
Cutoff:	570 nm
Emission:	590 nm
Sensitivity:	6 flashes/read or 200ms
PMT:	Auto
Auto calibrate:	On
Read:	Top
Read Height:	1*

*For microplate readers with Pre-Read Optimization option, the Read Height as well as Microplate Optimization is recommended before the first read.


13.9 Analyze the data as described below.

14. Calculations

- 14.1 Preconfigured protocols are available when using SoftMax Pro software from Molecular Devices
 - 14.2 Calculate the average fluorescence value for the blank control (zero) standards. Subtract the average blank control standard fluorescence value from all other fluorescence values.
 - 14.3 **Create a standard curve** by plotting the average blank control subtracted fluorescence value for each standard concentration (y-axis) against the target protein concentration (x-axis) of the standard. Use graphing software to draw the best smooth curve through these points to construct the standard curve.
- Δ **Note:** Most fluorescence reader software or graphing software will plot these values and fit a curve to the data. A four-parameter curve fit (4PL) is often the best choice; however, other algorithms (e.g. linear, semi-log, log/log, 4-parameter logistic) can also be tested to determine if it provides a better curve fit to the standard values.
- 14.4 Determine the concentration of the target protein in the sample by interpolating the blank control subtracted fluorescence **values against the standard curve**. Multiply the resulting value by the appropriate sample dilution factor, if used, to obtain the concentration of target protein in the sample.
 - 14.5 Samples generating fluorescence values greater than that of the highest standard should be further diluted and reanalyzed. Similarly, samples which measure at fluorescence values less than that of the lowest standard should be retested in a less dilute form.

15. Typical Data

Typical standard curve – data provided **for demonstration purposes only**. A new standard curve must be generated for each assay performed.

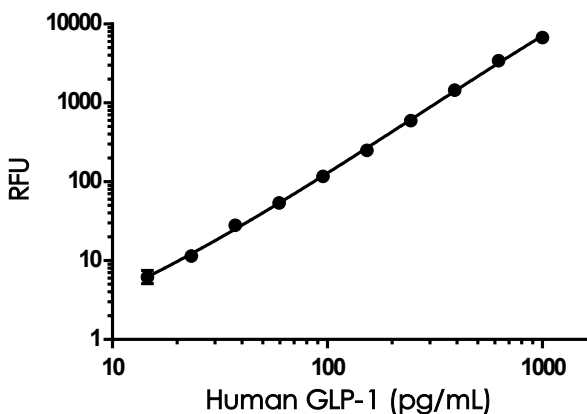

Standard Curve Measurements			
Concentration (pg/mL)	RFU		Mean RFU
	1	2	
0	25	25	25
14.6	30	32	31
23.3	36	37	36
37.3	54	51	53
59.6	79	79	79
95.4	136	148	142
152.6	279	271	275
244.1	600	646	623
390.6	1,486	1,475	1,481
625	3,445	3,480	3,462
1,000	6,792	6,753	6,772

Figure 1. Example of human GLP-1 (7-36) standard curve in Sample Diluent NS. The GLP-1 (7-36) standard curve was prepared as described in Section 10. Raw data generated on SpectraMax M4 Multi-Mode Microplate Reader is shown in the table. Background-subtracted data values (mean +/- SD) are graphed.

16. Typical Sample Values

SENSITIVITY –

The calculated minimal detectable dose (MDD) is 12 pg/mL. The MDD was determined by calculating the mean of zero standard replicates (n=12) and adding 2 standard deviations then extrapolating the corresponding concentration.

RECOVERY –

Three concentrations of GLP-1 (7-36) recombinant protein were spiked in duplicate to the indicated biological matrix to evaluate signal recovery in the working range of the assay.

Sample Type	Average % Recovery	Range (%)
10% Human Serum	109	105 – 112
10% Human Plasma - Citrate	115	107 – 123
1% Human Plasma - Heparin	110	104 - 112
10% Culture Media	99	93 – 102

Linearity of Dilution

Linearity of dilution is determined based on interpolated values from the standard curve. Linearity of dilution defines a sample concentration interval in which interpolated target concentrations are directly proportional to sample dilution.

Recombinant GLP-1 (7-36) was spiked into the following biological samples and diluted in a 2-fold dilution series in Sample Diluent NS.

Dilution Factor	Interpolated value	10% Human Serum	10% Human Plasma (Citrate)	1% Human Plasma (Heparin)	10% Culture media
Undiluted	pg/mL	257.70	260.90	265.20	238.00
	% Expected value	100	100	100	100
2	pg/mL	136.30	145.90	126.90	125.10
	% Expected value	106	112	96	105
4	pg/mL	68.60	73.40	67.60	60.50
	% Expected value	106	113	102	102
8	pg/mL	28.20	27.50	34.90	23.80
	% Expected value	87	84	105	80

PRECISION –

Mean coefficient of variations of interpolated values of GLP-1 (7-36) from three concentrations of human serum within the working range of the assay.

	Intra-Assay	Inter-Assay
n =	8	3
CV(%)	7	9

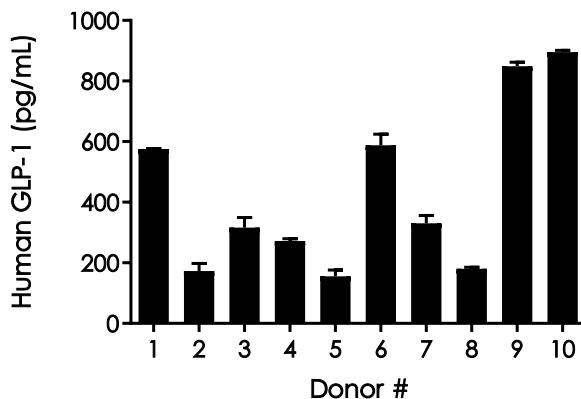


Figure 2. Ten individual healthy donors were evaluated for the presence of GLP-1 in serum using this assay. Serum of each donor was diluted 1:10 using sample diluent NS. The mean levels of GLP-1, after adjusting for dilution factor, were found at 433.5 pg/mL with a standard deviation of 277 pg/mL.

17. Assay Specificity

This kit recognizes both native and recombinant human GLP-1 (7-36) protein in serum, plasma, and culture supernatant samples.

CROSS REACTIVITY

GLP-1 (9-36) recombinant peptide was diluted at 10ng/mL and assayed for cross reactivity. Signal was found at 7% from GLP-1 (7-36) peptide assayed at the same concentration.

18. Species Reactivity

This kit recognizes human GLP-1 (7-36) protein.

Due to sequence similarity, this kit is predicted to cross react with multiples species such as mouse, rat, bovine, sheep, rabbit, pig and horse.

Please contact our Technical Support team for more information.

19. Troubleshooting

Problem	Reason	Solution
Poor standard curve	Inaccurate Pipetting	Check pipettes
	Improper standard dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low Signal	Incubation times too brief	Ensure sufficient incubation times; increase to 2 or 3 hour standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
	Incubation times with CatchPoint HRP Development Solution too brief	Read plate again after longer incubation time
Large CV	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions.
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	Store your reconstituted standards at -80°C, all other assay components 4°C. Keep Stoplight Red Substrate protected from light.
Precipitate in Diluent	Precipitation and/or coagulation of components within the Diluent.	Precipitate can be removed by gently warming the Diluent to 37°C.

20. Notes

Technical Support

Copyright © 2018 Abcam, All Rights Reserved. The Abcam logo is a registered trademark. All information / detail is correct at time of going to print. This product was released in collaboration with Molecular Devices LLC, however for technical support questions, please contact Abcam Representatives.

Austria

wissenschaftlicherdienst@abcam.com | 019-288-259

France

supportscientifique@abcam.com | 01.46.94.62.96

Germany

wissenschaftlicherdienst@abcam.com | 030-896-779-154

Spain

soportecientifico@abcam.com | 91-114-65-60

Switzerland

technical@abcam.com

Deutsch: 043-501-64-24 | Français: 061-500-05-30

UK, EU and ROW

technical@abcam.com | +44(0)1223-696000

Canada

ca.technical@abcam.com | 877-749-8807

US and Latin America

us.technical@abcam.com | 888-772-2226

Asia Pacific

hk.technical@abcam.com | (852) 2603-6823

China

cn.technical@abcam.com | +86-21-5110-5938 | 400-628-6880

Japan

technical@abcam.co.jp | +81-(0)3-6231-0940

Singapore

sg.technical@abcam.com | 800 188-5244

Australia

au.technical@abcam.com | +61-(0)3-8652-1450

New Zealand

nz.technical@abcam.com | +64-(0)9-909-7829